

1/13

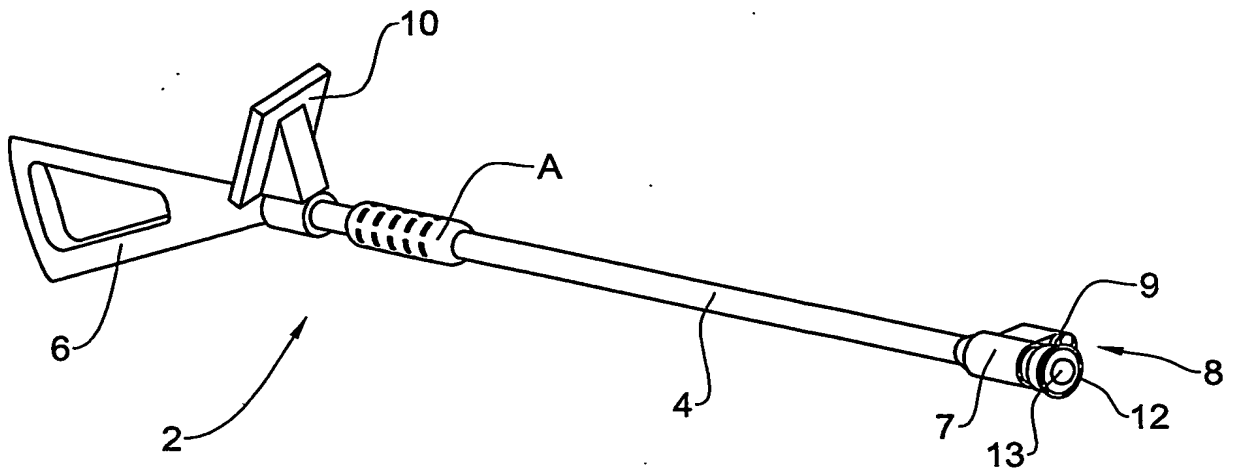


FIG. 1

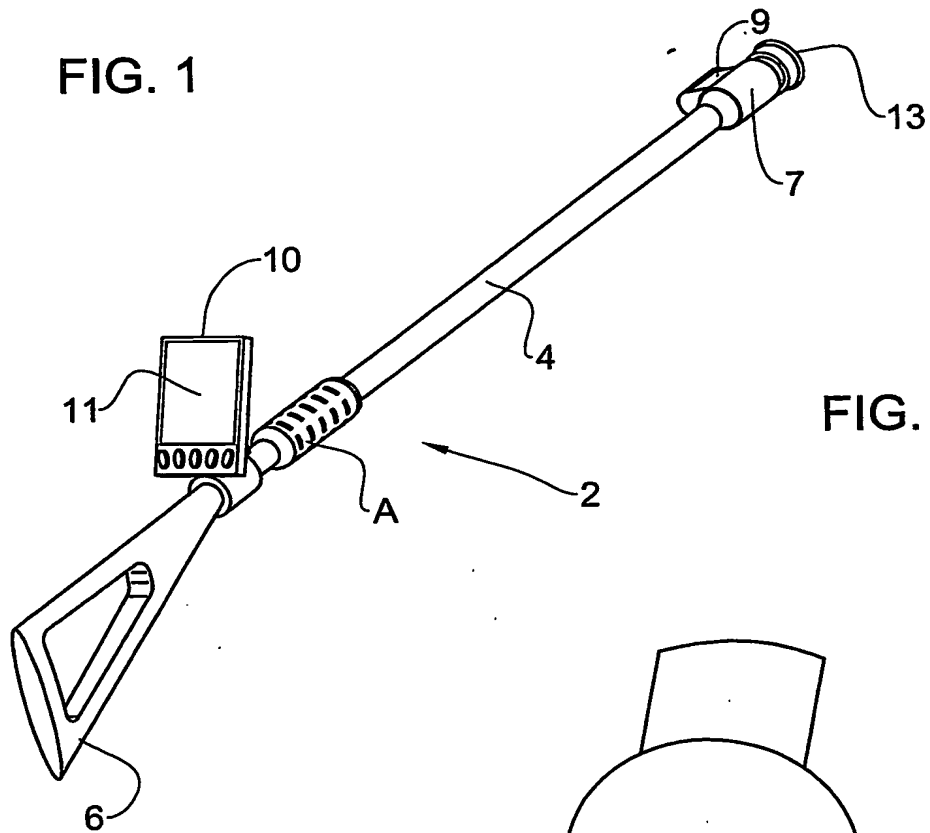


FIG. 2

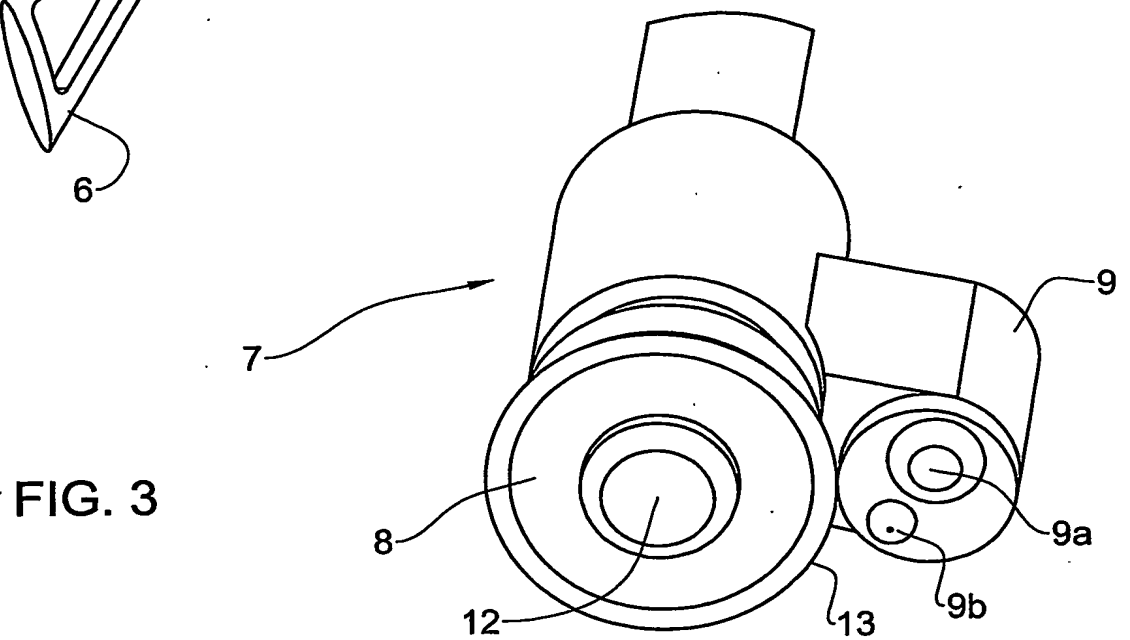


FIG. 3



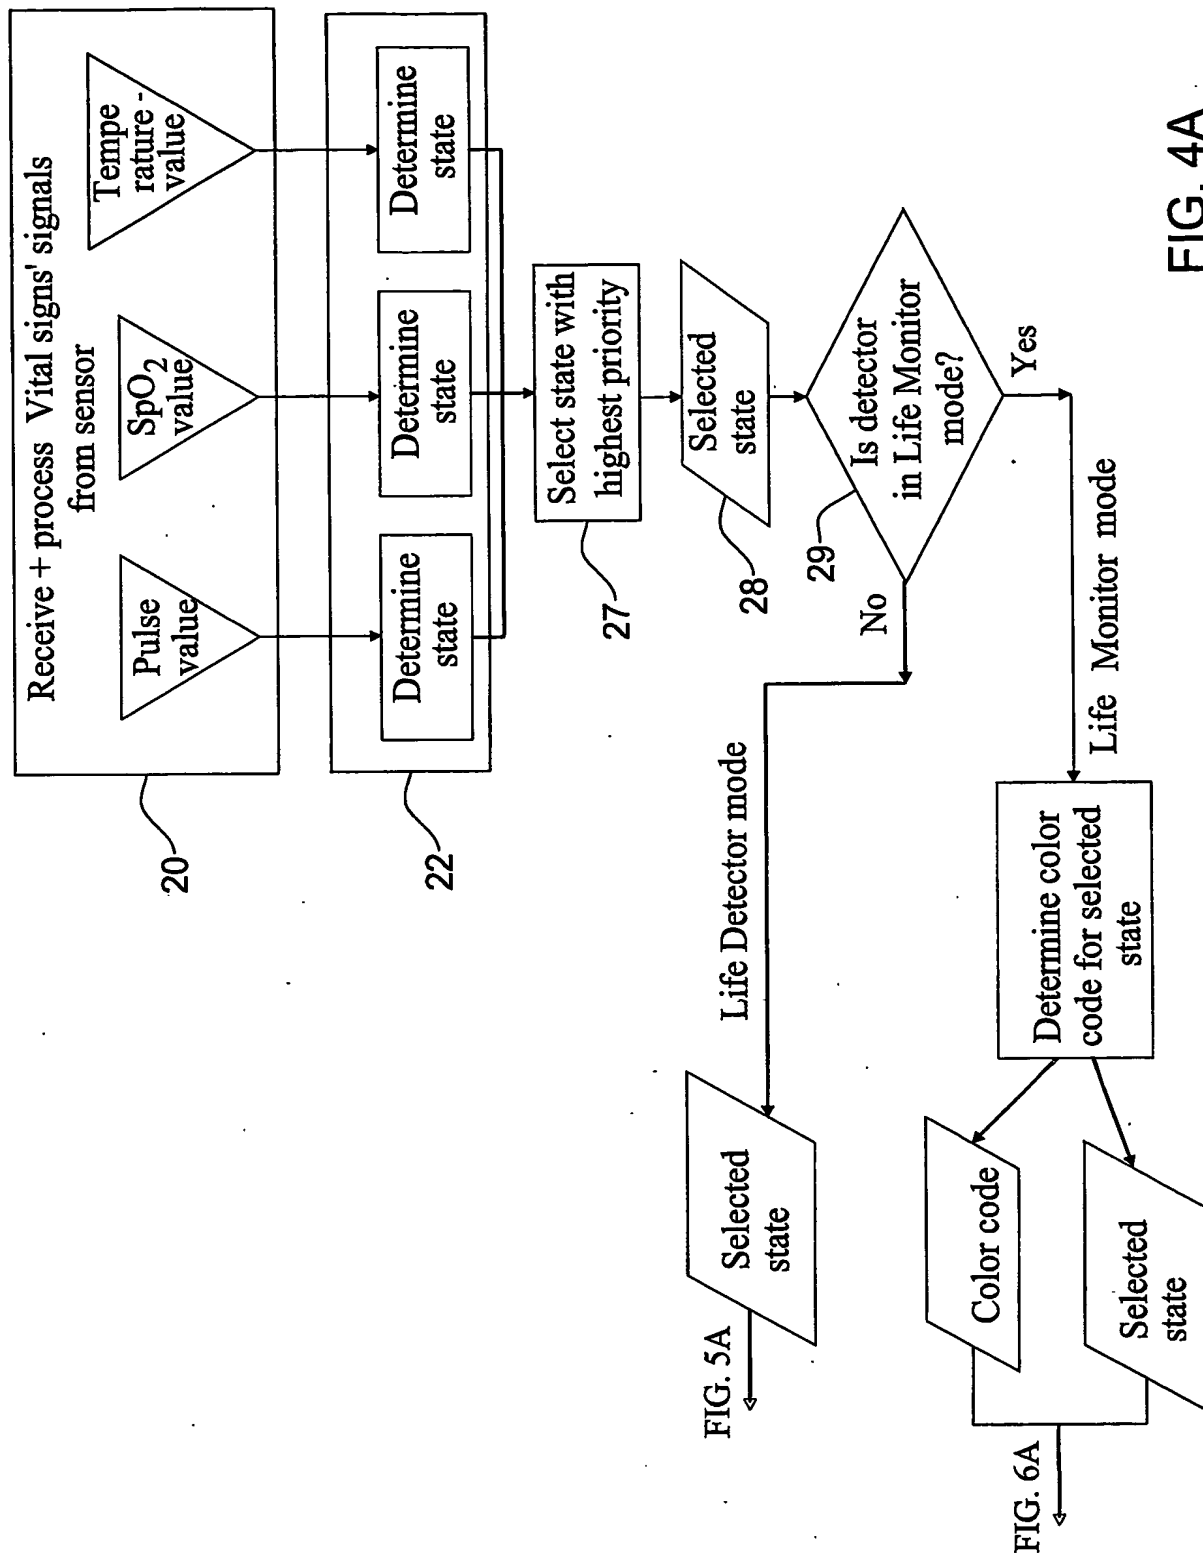


FIG. 4A

3/13

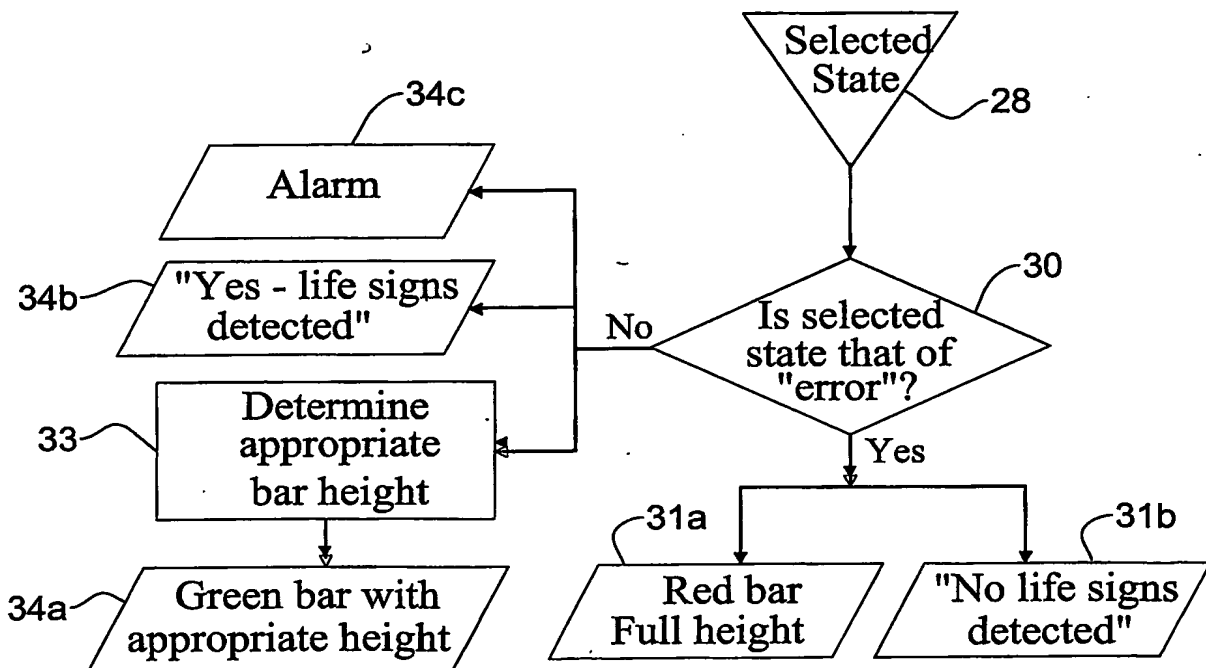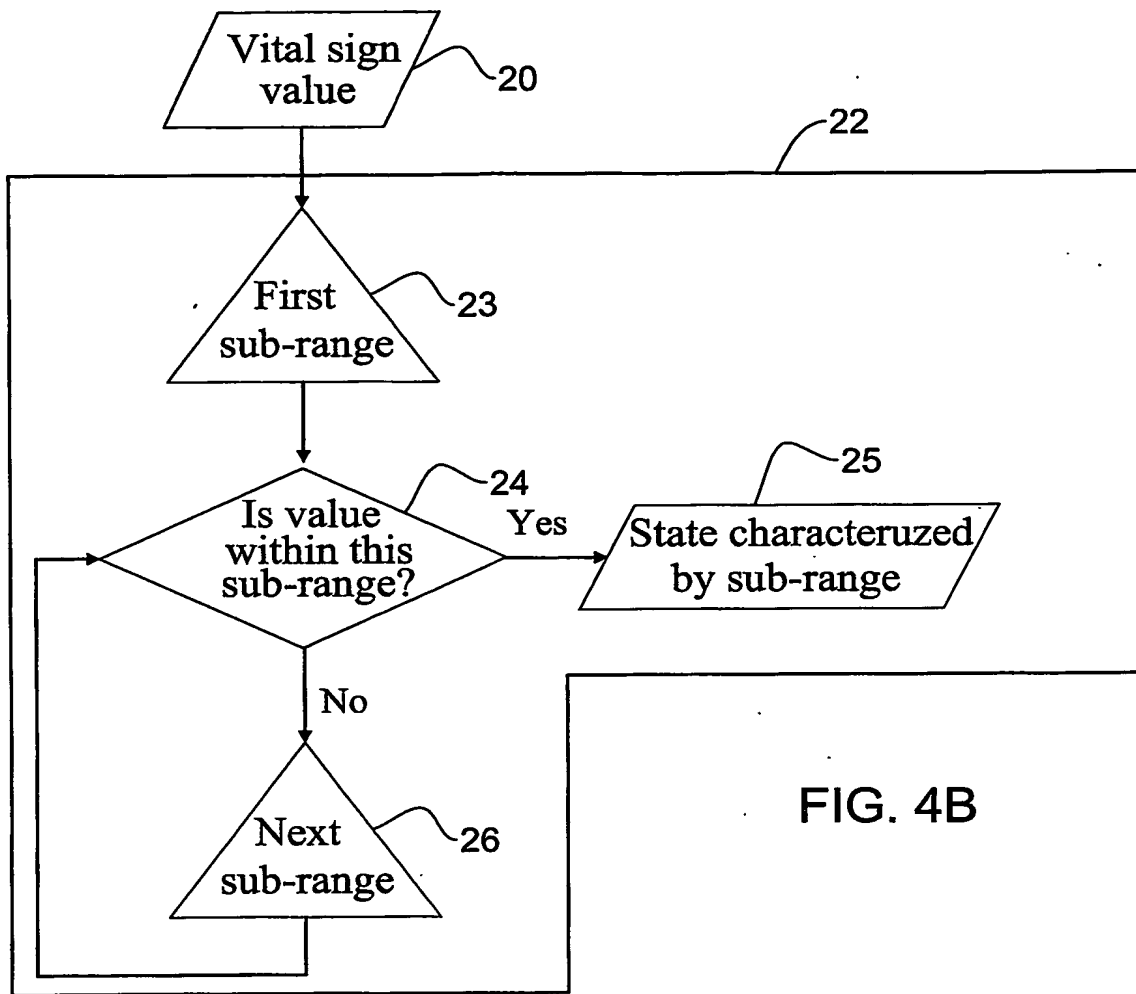

4/13

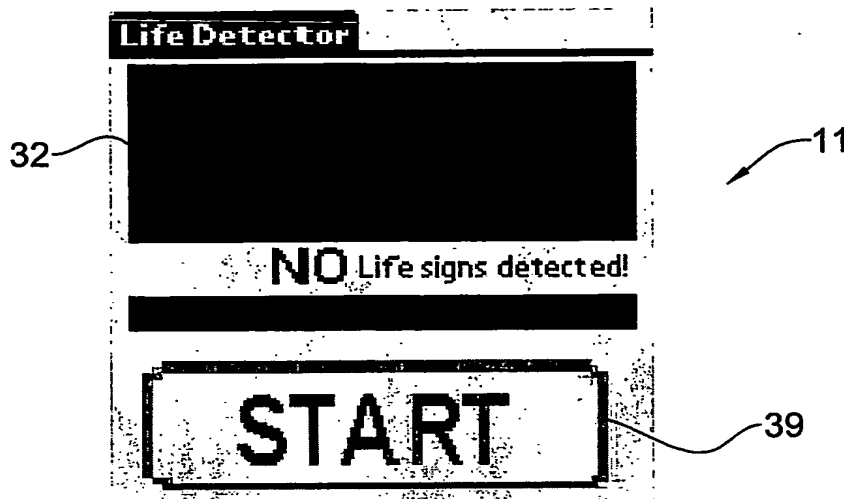


FIG. 5B

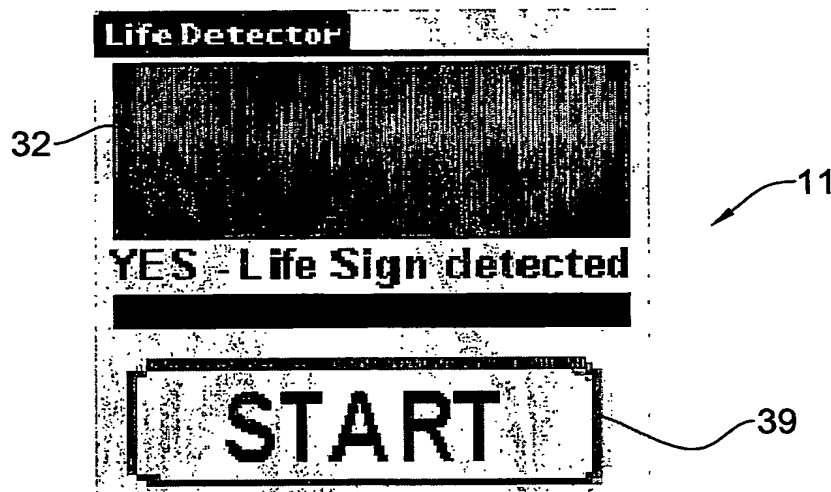


FIG. 5C

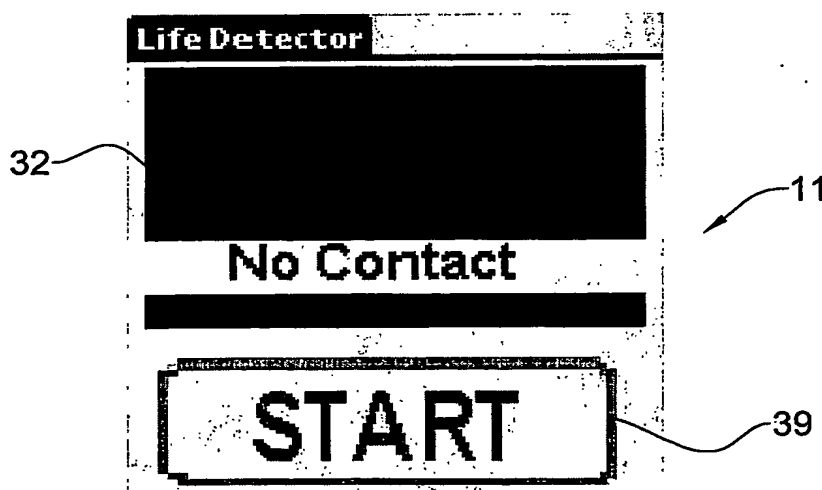


FIG. 5D

5/13

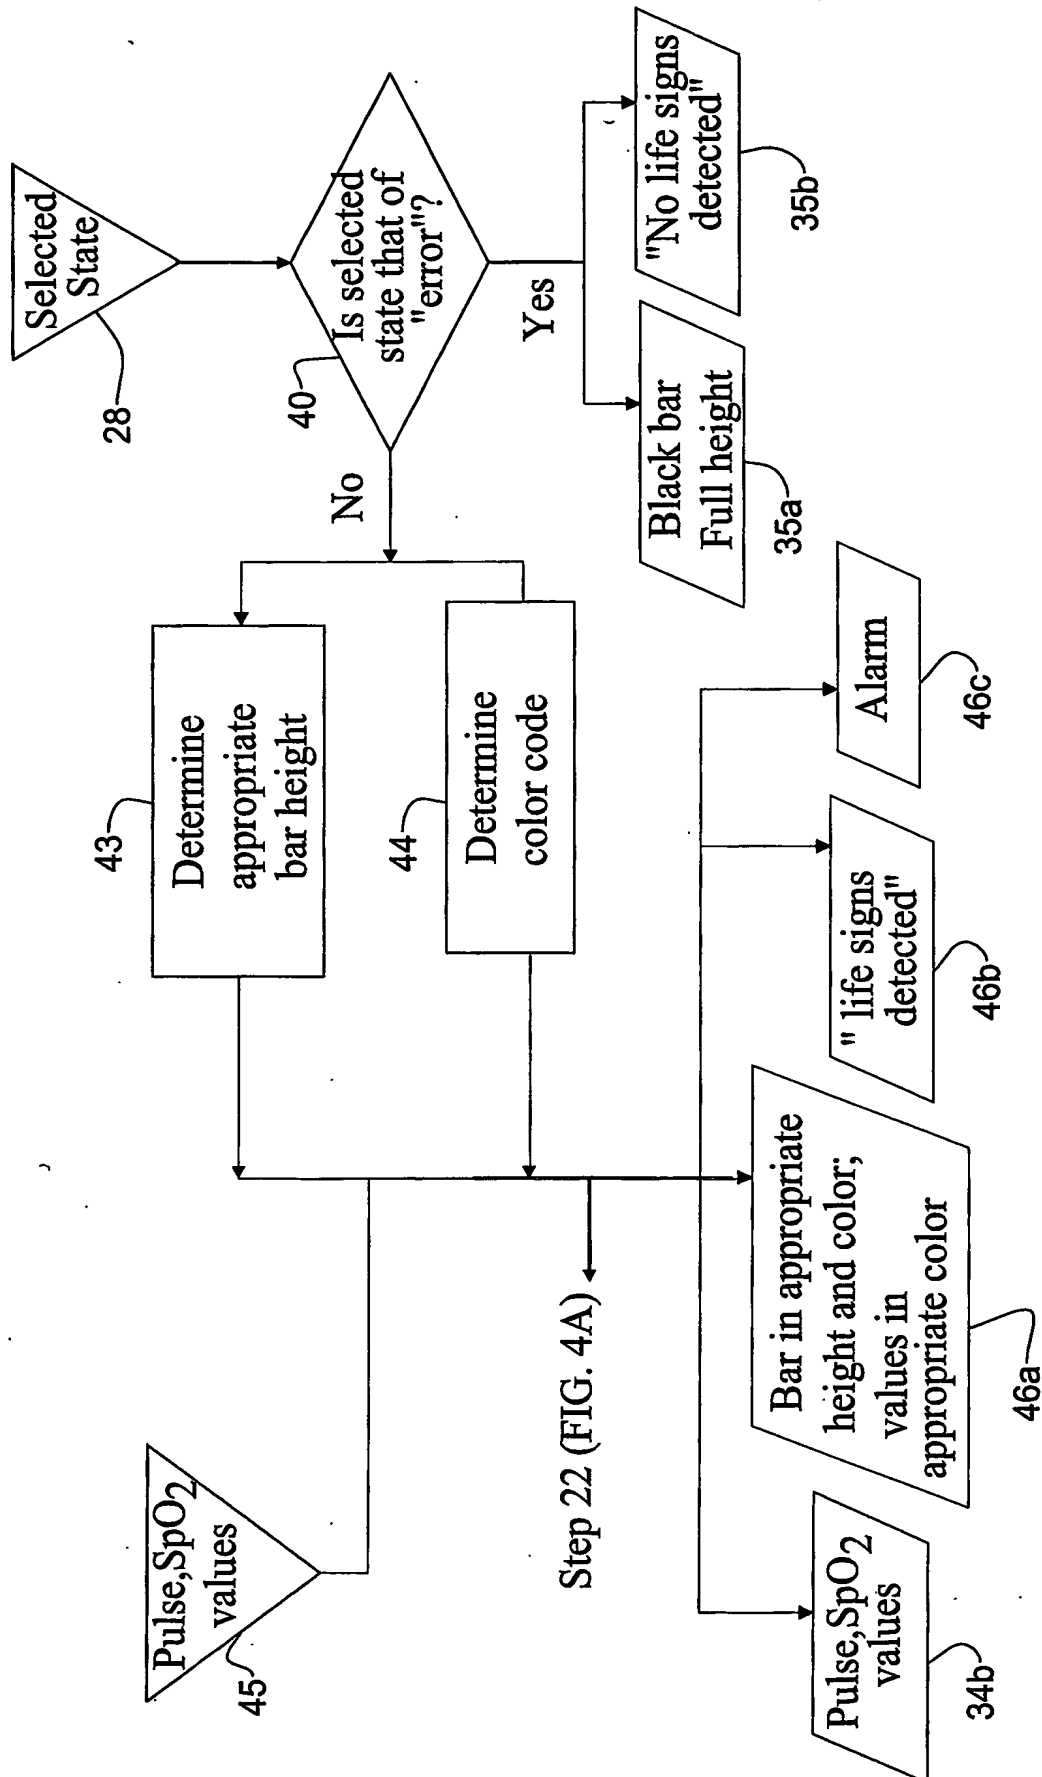


FIG. 6A

6/13

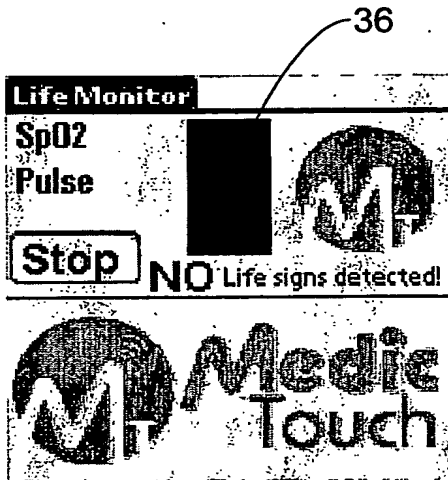


FIG. 6B

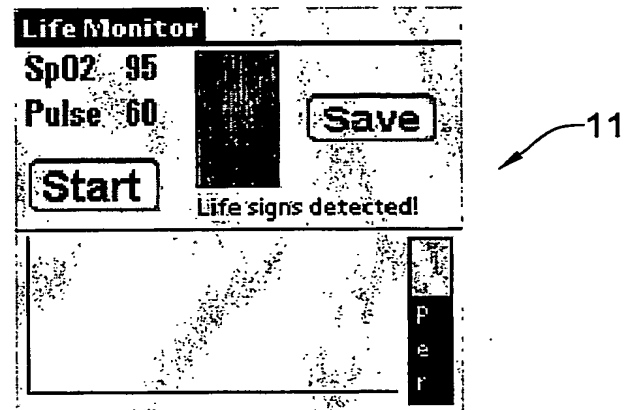


FIG. 6C

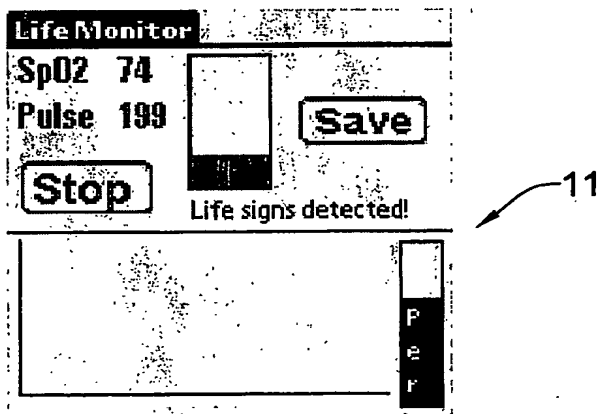


FIG. 6D

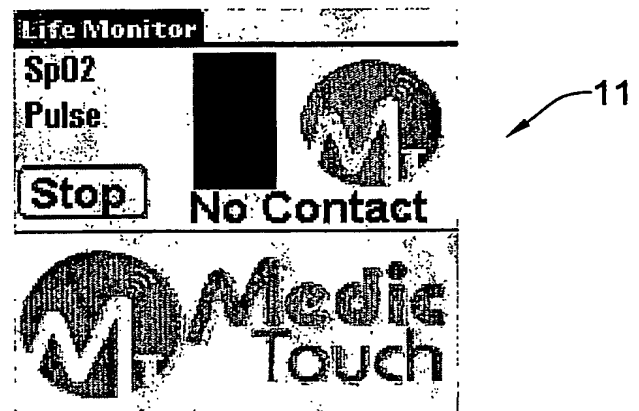


FIG. 6E

7/13



FIG. 8A

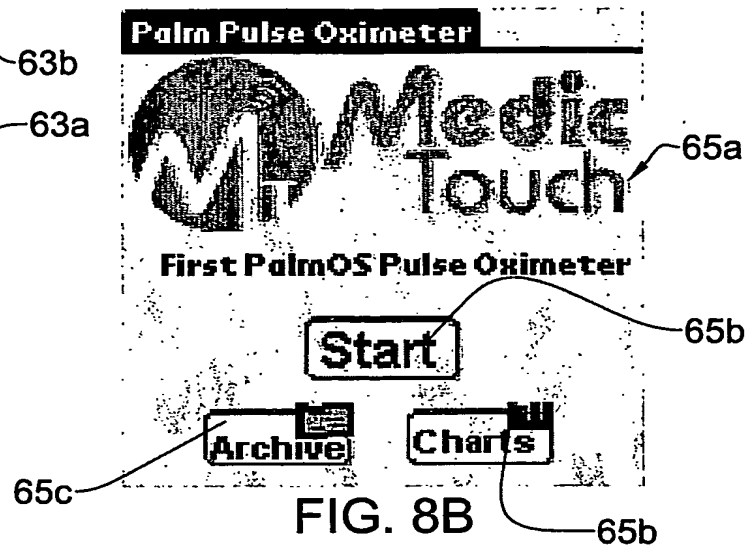


FIG. 8B

Counters	
No vital signs detected	267
High-Risk condition	4
Risk condition	22
Moderate condition	14
Normal condition	35
Total number checked	342
<input type="button" value="Done"/> <input type="button" value="Cancel"/> <input type="button" value="Reset"/> <input type="button" value="Send"/>	

FIG. 8C

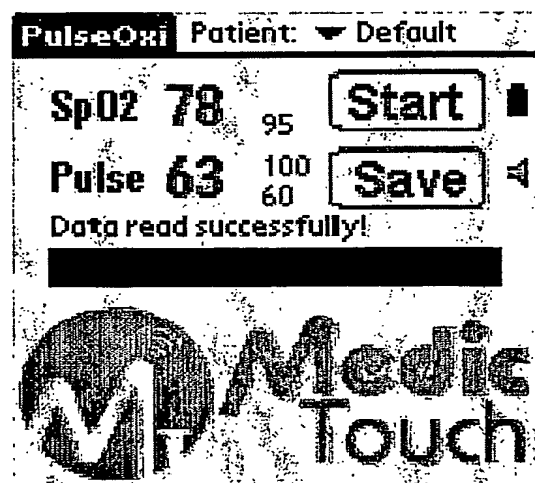


FIG. 8D

Measurements			▼ Default
Date	O2	Pulse	Notes
5/1/02 7:51	97	102	S
5/1/02 7:51	95	70	S
5/1/02 7:51	96	66	S
5/1/02 7:51	97	82	S
<div>Done New Edit Clear</div>			

FIG. 8E

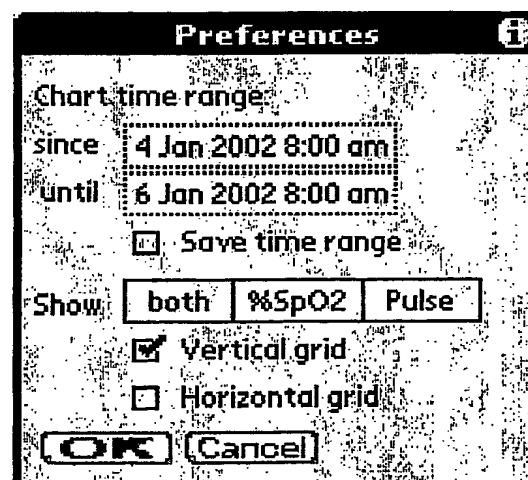


FIG. 8F

8/13

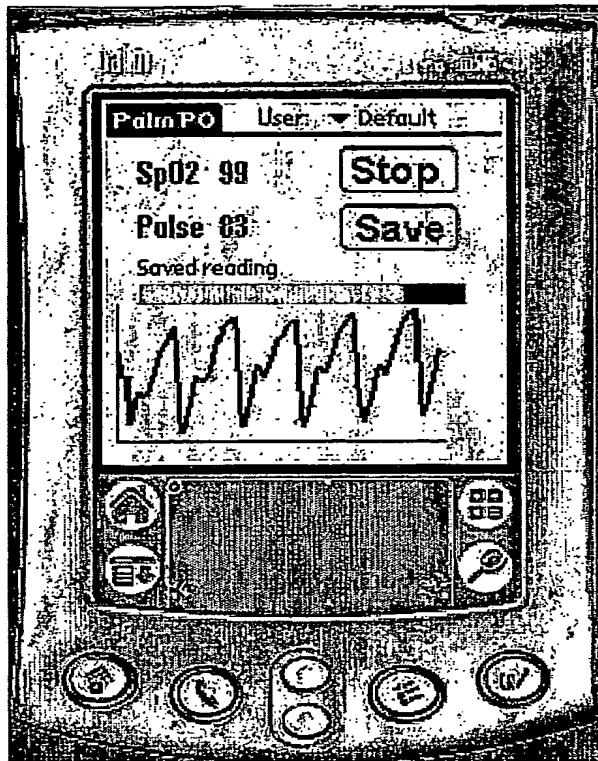


FIG. 8G

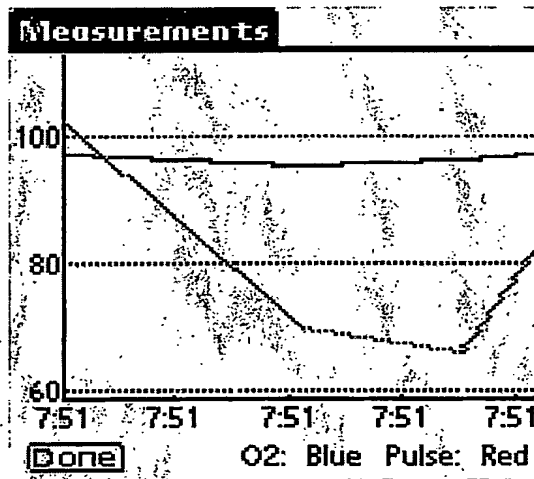


FIG. 8H

FIG. 8I is a screen titled 'Edit Patient'. It shows fields for Name, Pulse Alarm Above, Pulse Alarm Below, and SpO2 Alarm Below. The Name field is set to 'Default'. The Pulse Alarm Above is set to 100, and the Pulse Alarm Below is set to 60. The SpO2 Alarm Below is set to 95. There are 'OK' and 'Cancel' buttons at the bottom.

FIG. 8I

9/13

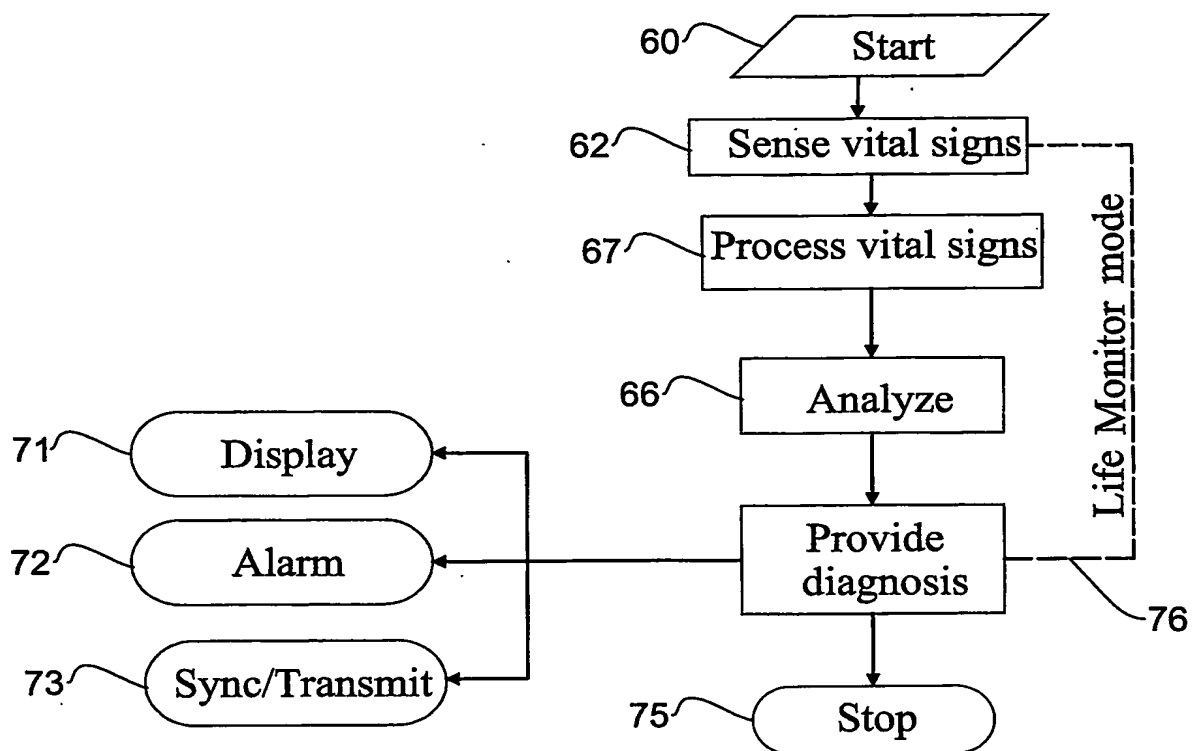


FIG. 7

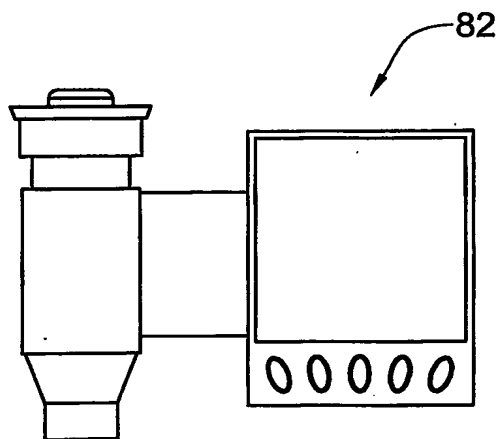


FIG. 9

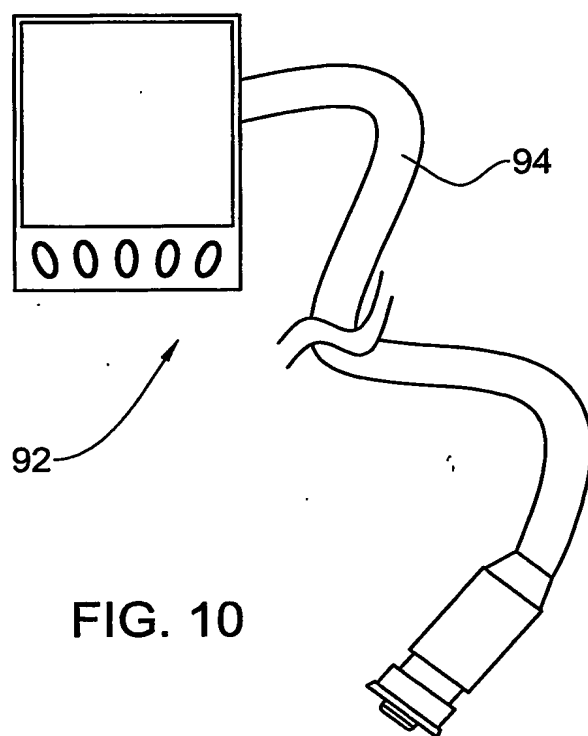


FIG. 10

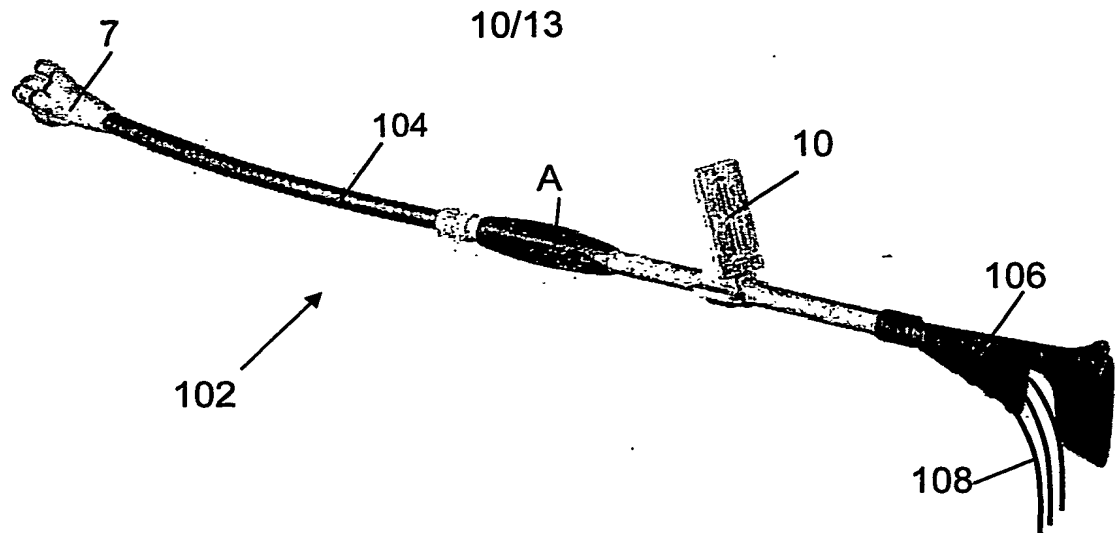


FIG. 11

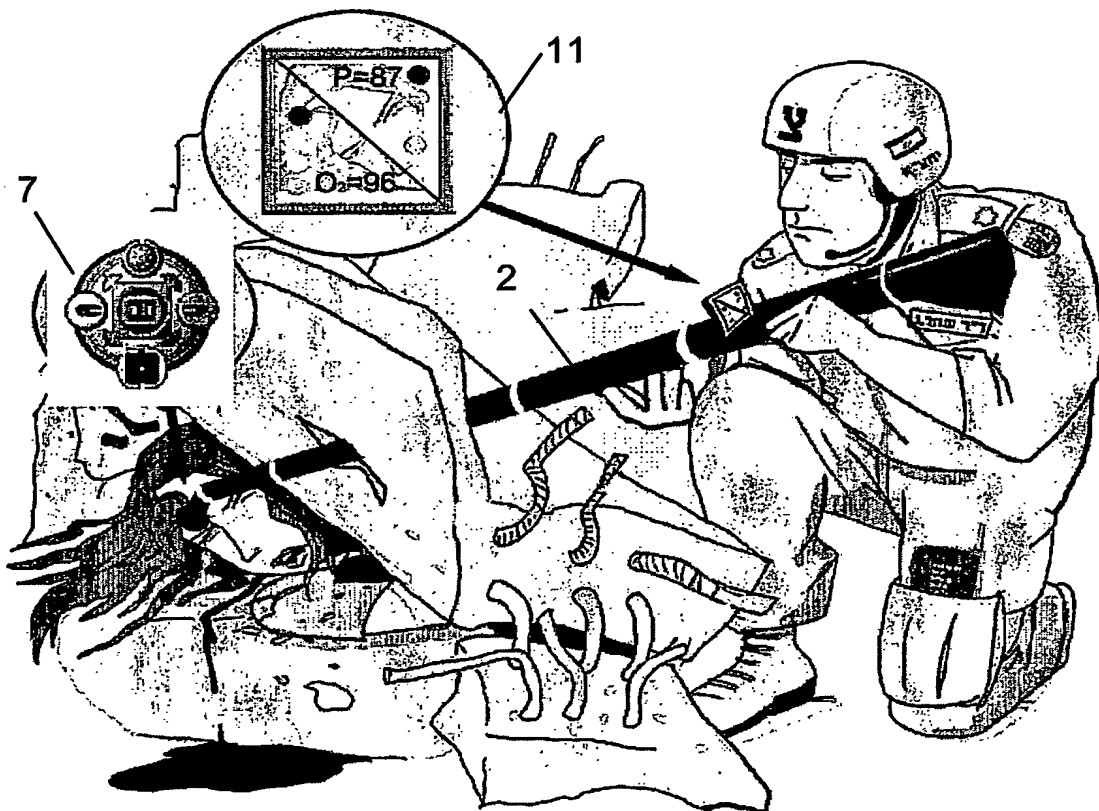


FIG. 12

11/13

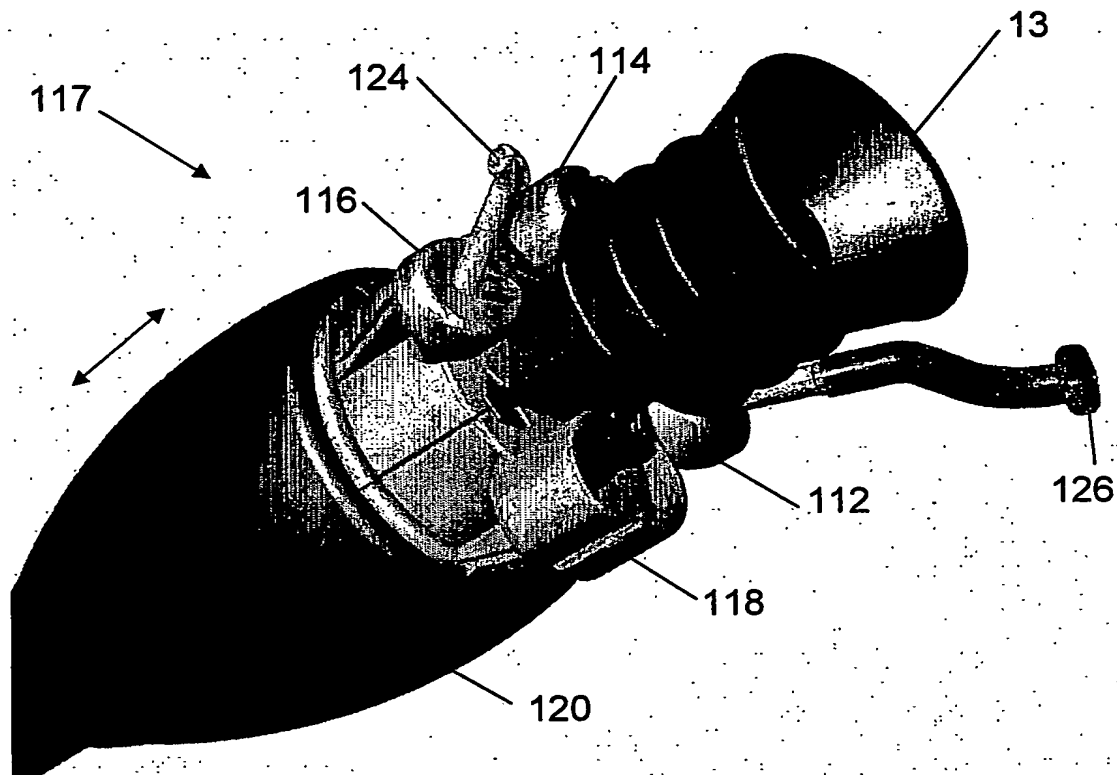


FIG. 13

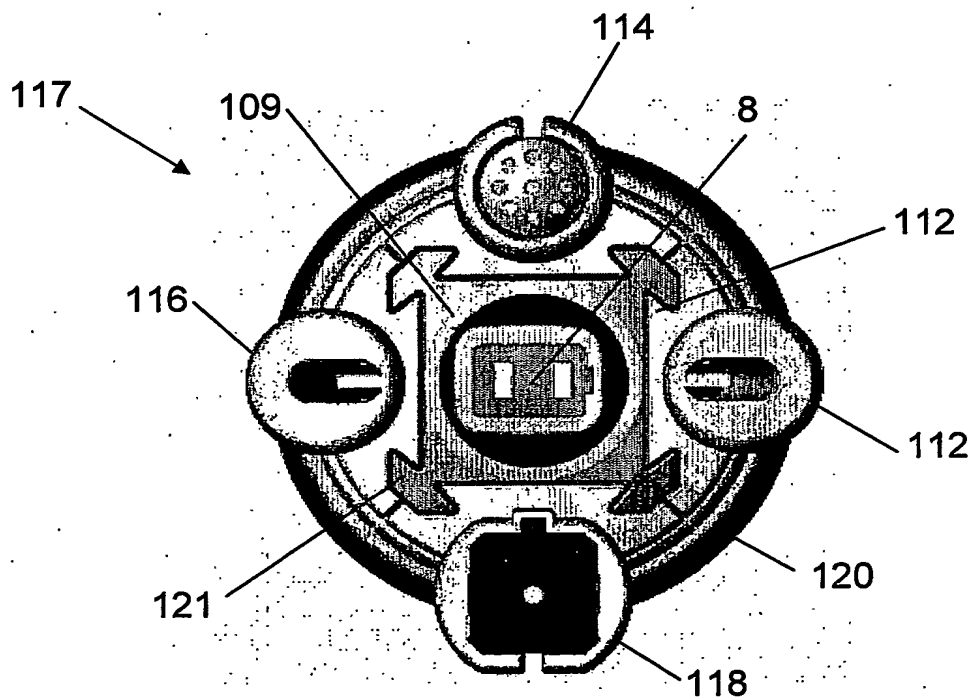


FIG. 14

12/13

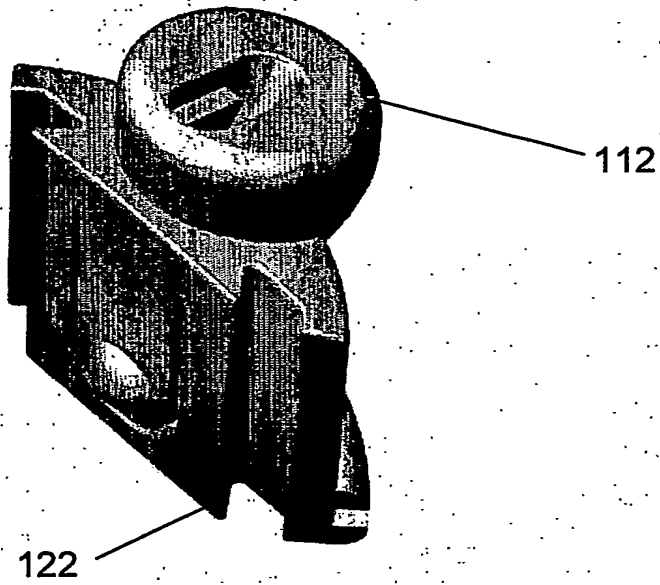


FIG. 15

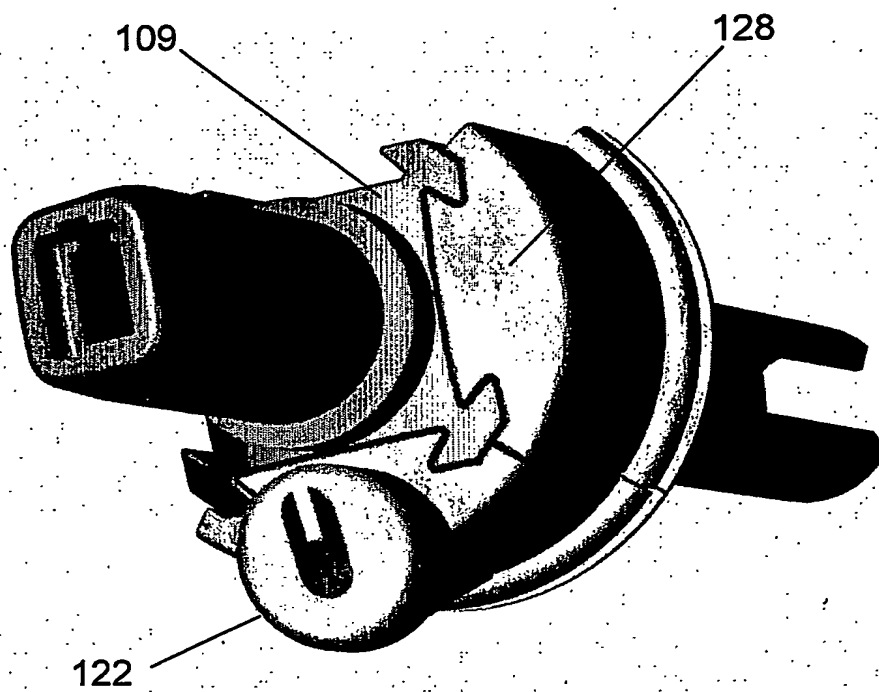


FIG. 16

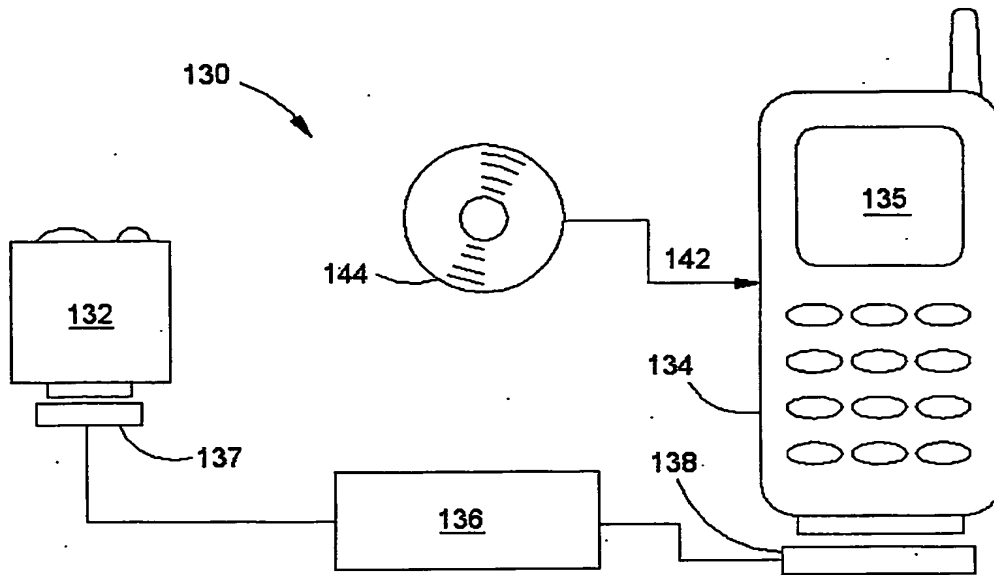


FIG. 17

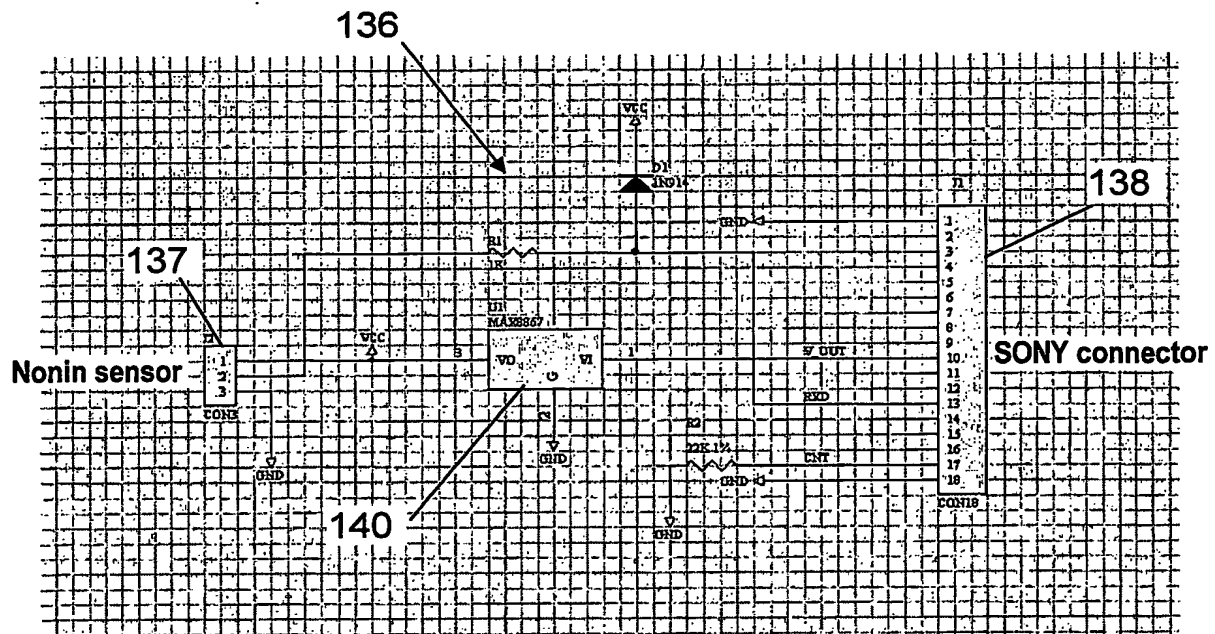


FIG. 18